

MAINTAIN YOUR VACUUM SYSTEM FOR LONGER LIFE WITH MONARCH CLEANSTREAM EVACUATION SYSTEM CLEANER



CleanStream



 Monarch.

by

AIR
TECHNIQUES equipped for life®

DAILY CLEANING WITH MONARCH CLEANSTREAM

Monarch CleanStream cleans, deodorizes and maintains your evacuation lines optimizing system performance and keeping your vacuum system running smoothly. We recommend cleaning each operatory once a day or more often if deemed necessary due to the procedure such as extractions, periodontal therapy, or the removal of sticky resin restorations. *To ensure best cleaning results, please follow instructions below.*

1 DOSAGE 2% DILUTION - MIX & SHAKE



1 Liter



2 Liters



1 operatory: Mix 1 liter of water + 1 cap of Monarch CleanStream (20 ml) – shake lightly

2 operatories: Mix 2 liters of water + 2 caps of Monarch Cleanstream (40 ml) – shake lightly

2 CLEANING OF EVACUATION LINES – ASPIRATE



Operatory 1: Place Vortex Dispenser in upright position. Attach hoses, open handpiece valves, aspirate 1 liter per operatory (*stops automatically after 1 liter is aspirated; no monitoring needed*)


Operatory 2: Place Vortex Dispenser in horizontal position. Dispense the rest of the solution.

3 CLEANING OF CUSPIDOR (OPTIONAL)



A minimum of 250 ml of diluted CleanStream solution per cuspidor

4 DURATION TIME

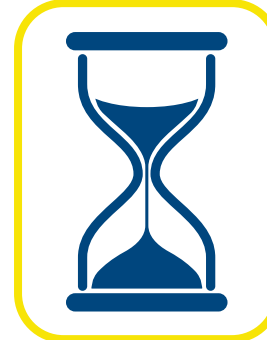

Ideally leave solution in evacuation lines for at least one hour or overnight.

5 FLUSH (OPTIONAL)



For best cleaning results, flush lines with 2 liters of water after the exposure time or the next morning prior to patient care.